

Hardline Laboratory

Report No. : HL90581/2020

Page : 1 of 2

Date : OCT. 20, 2020

INTERWORLD NETWORK (M) SDN BHD

G-11 & G-12, KOMPLEKS SEMPILAI, JALAN SEMPILAI, 13700 SEBERANG JAYA,
PENANG, MALAYSIA

The following merchandise was submitted and identified by the applicant as:

Product Description: 3 PLY SURGICAL MASK

We have tested the submitted sample(s) as requested and the following results were obtained:

Test Requested: ISO 22609:2004


Test Method & Result: ---See following sheet(s)---

Date of Receipt: SEP. 26, 2020

Testing Period: SEP. 26, 2020 ~ OCT. 20, 2020

Note: This testing was performed by O.S.H. CO., LTD. Respirator Test Center.

Signed for and on behalf of
SGS Taiwan Ltd.


Sturm Su
Asst. Manager



This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.tw/Terms-and-Conditions> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.tw/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of client's instruction, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced, except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested.

Test Method & Result:

Test Methods	Test Item		Test Article Number	Synthetic Blood Penetration
1. Testing Sample Number: 32 2. Test Side: Outside 3. Pre-Conditioning : Minimum of 4 hours at (21±5) °C and (85±5) % relative humidity (RH) 4. Test Conditions : 28.4 °C and 35.2 % RH 5. Sample Model: SBP-1090929003	Synthetic Blood Penetration Resistance	120 mmHg (16.0 kPa) As per client requested	01-07、 09-12、14-23、 25-32	None Seen
			8、13、24	Yes

Note :

1. The test report merely reflects the test results of the consigned matters of the client and is not a certification.
2. The content of this report is invalid if it is not presented as the entire report.

- Picture(s) -

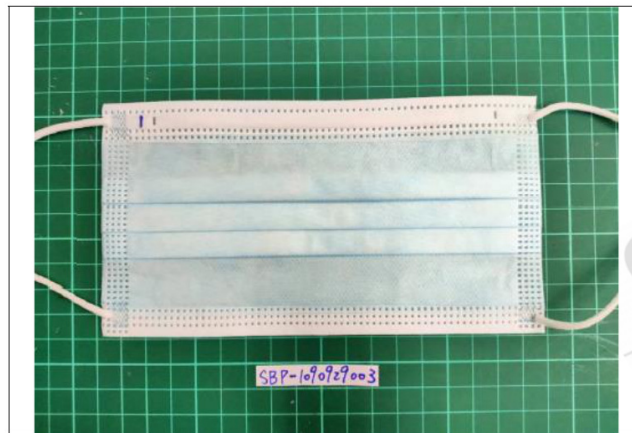


Photo A: Appearance of the sample
- SBP-1090929003

---End of Report---