

Hardline Laboratory

Report No. : HL90580/2020

Page : 1 of 2

Date : OCT. 20, 2020

### INTERWORLD NETWORK (M) SDN BHD

G-11 & G-12, KOMPLEKS SEMPILAI, JALAN SEMPILAI, 13700 SEBERANG JAYA, PENANG, MALAYSIA

#### The following merchandise was submitted and identified by the applicant as:

Product Description: 3 PLY SURGICAL MASK

#### We have tested the submitted sample(s) as requested and the following results were obtained:

Test Requested: EN 14683:2019 Annex C


Test Method & Result: ---See following sheet(s)---

Date of Receipt: SEP. 26, 2020

Testing Period: SEP. 26, 2020 ~ OCT. 20, 2020

Note: This testing was performed by O.S.H. CO., LTD. Respirator Test Center.

Signed for and on behalf of  
SGS Taiwan Ltd.

  
Sturm Su  
Asst. Manager



### Test Method & Result:

Test Methods	Test Item	Test Results (mm H <sub>2</sub> O/cm <sup>2</sup> )	Test Results (Pa/cm <sup>2</sup> )	
1. Testing Sample Number: 5 2. Test Flow Rate : 8.00 Liter/min 3. Pre-Conditioning: Minimum of 4 hours at (21±5) °C and (85±5) % relative humidity. 4. Sample Model: AEP-1090929003	Differential pressure	01	5.83	57.13
		02	5.50	53.90
		03	5.87	57.53
		04	5.06	49.59
		05	5.00	49.00
		Avg.	5.45	53.43

### Note :

- The test report merely reflects the test results of the consigned matters of the client and is not a certification.
- The content of this report is invalid if it is not presented as the entire report.

– Picture(s) –

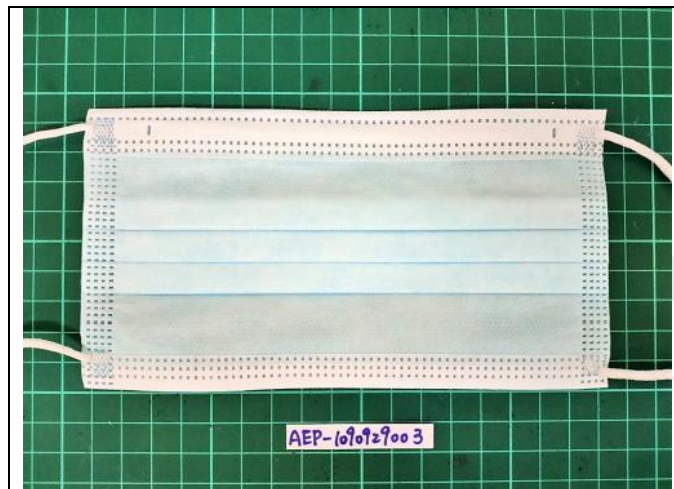


Photo A: Appearance of the sample  
- AEP-1090929003

---End of Report---